

***KEMKRAFT* ENGINEERING, INC.**
MODEL KEI-200/BS SPC DIGITAL INCLINOMETER

***KEMKRAFT* ENGINEERING, INC.**
INSTRUCTIONAL MANUAL


SPC DIGITAL INCLINOMETER
MODEL KEI-200/BS
W/ OPTIONAL BARCODE SCANNER

REVISION DATE:

SEPT. 19 1997

KEMKRAFT ENGINEERING, INC.

MODEL KEI-200/BS SPC DIGITAL INCLINOMETER

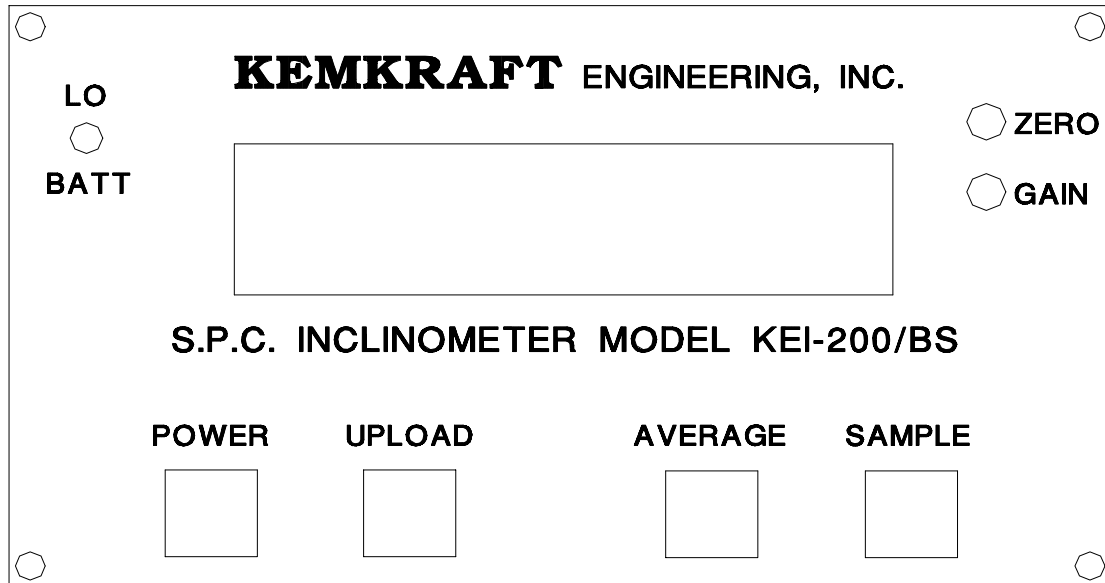

OPERATION PROCEDURE:

- This unit should be calibrated **once a week minimum**. Refer to the **Calibration Procedure** of this manual.
- The Inclinometer should be fully charged before use. If the unit is used extensively during the day it should be charged at night.
- Depress the power switch, located on the front panel, to turn the unit on. The unit should display as follows:

XX.Xdeg XXXsmpl
 avg XXXavct

XX.Xdeg displays the degree angle value up to a max. of +/-17.5 deg.

smpl: is the sample counter and indicates the amount of samples stored into the units' memory. Maximum samples: 249

avg: is the abbreviation for average and will display the average value of the sum of the samples taken when the SAMPLES button is depressed.

avct: is the abbreviation for average counter and will display the amount of averages stored into the units memory each time the AVERAGE button is depressed. Maximum Average count: 250

KEMKRAFT ENGINEERING, INC.

MODEL KEI-200/BS SPC DIGITAL INCLINOMETER

Mount the mechanical fixturing accurately onto the vehicle steering wheel. Tests performed should be done on the flattest, smoothest road possible and starting and stopping points should be noted. Drive the vehicle at a slow, constant speed and at the starting point depress the SAMPLE button. The sample counter will automatically up count. **(When the sample button is pushed at the beginning of the first and second pass, a one second delay timer has been added 11-20- 93 to give the driver a second to straighten the vehicle.)** When the stopping point is reached, depress the SAMPLE button again and the sample taking will cease. Turn the vehicle around and drive at the same constant speed as was in the opposite direction. When the vehicle reaches the previous point that the SAMPLE button was pressed to stop the sampling, press the SAMPLE button again. The sample counter will automatically down count and stop when it reaches 000 SAMPLES. If the test was performed without any flaws, and the values taken you felt were accurate, depress the AVERAGE button. This will display, in front of AVG, the average value of the sum of samples taken and also display in front of AVGCT the amount of averages saved for future uploading. When the tests are complete and averages have been stored into the units memory, the unit can than be turned off and taken to a computer that has a serial port.

RS-232-C SERIAL UPLOAD PROCEDURE

Plug the interface cable supplied with the inclinometer into the side of the unit. Plug the 9 pin computer interface connector into the serial port of the computer. Turn the inclinometer back on and notice that the average counter reads the same amount of samples when the unit was turned off. The Kemload Utility Program that was supplied with the inclinometer can be run by typing KEMLOAD <CR>. This will display on the computer CRT the Kemload program. Depress on the inclinometer the UPLOAD button and the display will read, RS232 SRL UPLOAD, XXX AVRGS STORED. The average values are now ready for upload to the computer. The Kemload Utility Program on the CRT displays the function keys of an IBM-AT keyboard at the bottom of the screen. View these function key commands and press the appropriate keys. To upload the averages in the inclinometer, press the F6 key and the average values taken during the tests will be displayed on the screen. A file name should be assigned to that set of data by using the F4 key for changing the file name. By pressing the F2 key the values displayed on the CRT are then saved in an ASCII text file under the name that you assigned.

KEMKRAFT ENGINEERING, INC.

MODEL KEI-200/BS SPC DIGITAL INCLINOMETER

CALIBRATION PROCEDURE:

- Charge unit over night before calibrating.
- Install mechanical steering wheel fixture (with inclinometer permanently mounted onto it) onto a calibration stand that can be adjusted for 0 degrees and some other known value such as 5 or 10 degrees.
- Set the cal. stand to 0 degrees and adjust the ZERO control on the front panel of the inclinometer for 00.0 degrees.
- Set the cal. stand to eg. 10 degrees and adjust the GAIN control on the front panel of the inclinometer for 10.0 degrees.
- Repeat the following two procedures until the values are stable.

WARRANTY AND SERVICE INSTRUCTIONS

KEMKRAFT Engineering, Inc. warrants this equipment against defects in workmanship and materials for a period of 90 days from date of signature of release. We will, at our option, repair or replace products which prove defective during the warranty period. No other warranty, expressed or implied, is given. KEI is not liable for consequential damages. Damage caused to the equipment as a result of improper use or abuse, or unauthorized modification of the instrument is not covered under this warranty.

For service contact: KEMKRAFT Engineering, Inc.
47650 Clipper Dr.
Plymouth Twp., MI. 48170

(734) 414-6500

KEMKRAFT ENGINEERING, INC.

MODEL KEI-200/BS SPC DIGITAL INCLINOMETER

Barcode SCANNER Option

The KEI-200/BS was developed to allow the user to scan a Vehicle Identification Number (VIN) of the vehicle that is being audited. This allows the VIN to be stored along with the drive audit average for the vehicle. This information can be uploaded to a P.C. for S.P.C.

OPERATION

The KEI-200/BS is designed to have the scanner plugged directly into the 9 pin serial port.

- 1). This port provides power and communication to barcode scanner.
- 2). This port is also used to upload the stored audit data.

Plug the barcode scanner into the serial port.

Depress the power switch, located on the front panel, to turn the unit on. The barcode scanner will beep to confirm powerup. The unit should display the following:

XX.Xdeg XXXsmpl
avg XXXavct

Direct the scanner head at the desired build sheet VIN and press the trigger. The scanner will emit a visible RED horizontal beam. This beam scans the barcode. When the scanner has a good scan, a green LED on the unit will blink and the unit will beep. The KEI-200/BS should display the following:

VIN XXXXXXXXXX
press SAMPLE sw.

Press the **SAMPLE** switch to continue with the barcode Audit.

The unit should display the following:

SAMPLE = Accept
AVERAGE = Reject

Press the **SAMPLE** switch to apply the scanned VIN to the next Drive Audit Data, the KEI-200/BS is now ready for a Drive Audit. (Refer to Drive Audit operation procedure)

Press the **AVERAGE** switch to apply the scanned VIN to the previous Drive Audit Data.